







# CATHCHECK™ SYSTEM

Instant epidural catheter verification  
with CompuWave™ Display graphing  
the pulsatile waveform found in the  
epidural space.




\*Catheter and adaptor sold separately

## Benefits

-  Saves the anesthesia provider time, enabling them to make clinical decisions faster
-  The anesthesia provider may flush with sterile anesthetic or sterile saline
-  Increases the anesthesia provider's daily effectiveness
-  Provides confirmation to the anesthesia provider post-catheter placement
-  Reduces the amount of time the patient is in pain, due to an ineffective catheter
-  The CompuWave™ Display shows the pulsatile waveform found in the epidural space, again confirming needle and catheter placement

## See the Difference

### CATHETER DOSING VS. CATHCHECK SYSTEM

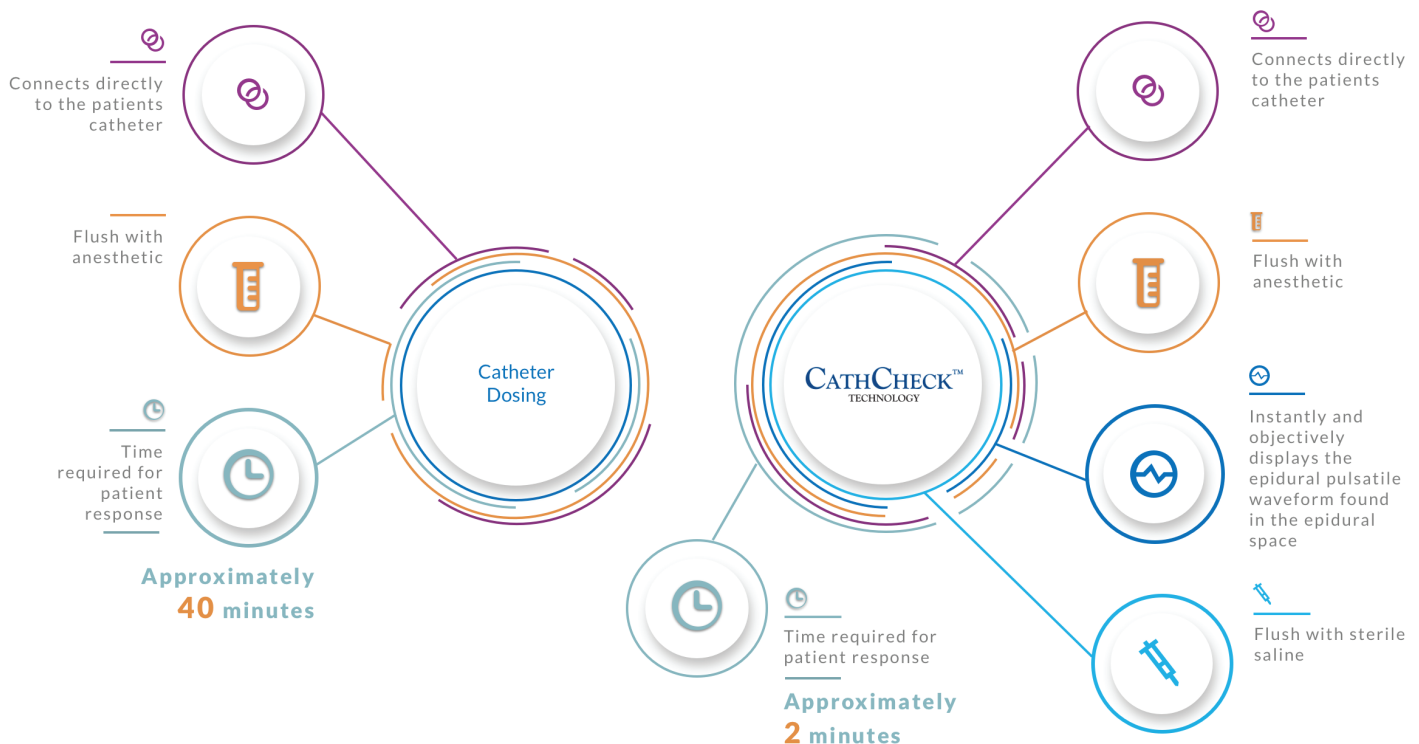

# Specifications & Order Information

\*Catheter and adaptor sold separately

## CompuFlo® Epidural Instrument Specifications

Voltages	100-264 V, 50/60 Hz
Internal Battery	Up to 2 hrs of use
Weight	2.3 kg (5.0 lbs)
Dimensions	24.38 x 17.15 x 14 cm (9.6 x 6.75 x 5.5 in)
Operational Temperature	10-35 °C (50-95 °F)
Operational Humidity	30-70% RH
Storage Temperature	-20-45 °C (-4-113 °F)
Storage Humidity	15-90% RH
Compliance	<p>IEC 60601-1 3.1 (2012) Edition "Medical electrical equipment - Part 1: General requirements for basic safety and essential performance"</p> <p>"Medical Electrical Equipment: Part 1-2 General Requirements for Basic Safety and Essential Performance Collateral Standard: Electromagnetic Compatibility Requirements and Test"</p>

## CompuFlo® Instruments Specifications

CompuFlo® Epidural Instrument 110	EPI-6000-110
CompuFlo® Epidural Instrument 220	EPI-6000-220

## CathCheck™ Equipment

CathCheck™ ID Adaptor & Kit	EPI-6010-03
-----------------------------	-------------

## CompuFlo® Instruments

CompuFlo® Epidural ID Adaptor & Kit	EPI-6010
-------------------------------------	----------